







YOU CAN DO IT

WITHOUT LANCETS²




With the FreeStyle LibreLink app,¹ you can scan your FreeStyle Libre 2 sensor with an iPhone

Downloading the FreeStyle LibreLink app¹

-  Go to **App Store**
-  Search FreeStyle LibreLink
-  Look for FreeStyle LibreLink – UK
-  Press **Get**
-  Install by entering your Apple ID (the app is free to download and use)
-  Once downloaded open the app and follow the on-screen instructions to get set-up


Scanning the FreeStyle Libre 2 sensor with an iPhone

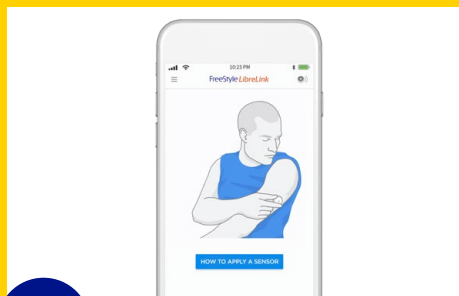

- 1** First open the FreeStyle LibreLink app on your iPhone and tap the **scan** button



- 2** Hold the **top of the iPhone** near the sensor

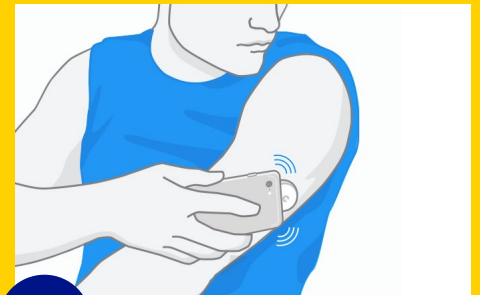

- 3** Do not move your iPhone until you **hear a tone** and/or feel a vibration. This completes the scan

ALARM. SCAN. ACT


Quick Tips

- The Near Field Communication (NFC) antenna on an iPhone is on the top edge.
- Remove bulky or metallic phone cases as they can interfere with the NFC signal.


Visit www.FreeStyleDiabetes.co.uk for more information

The FreeStyle LibreLink app and your iPhone



It's easy to set alarms on your FreeStyle LibreLink app

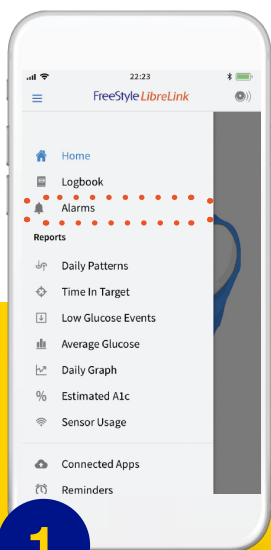


1 Tap Alarms in the menu³

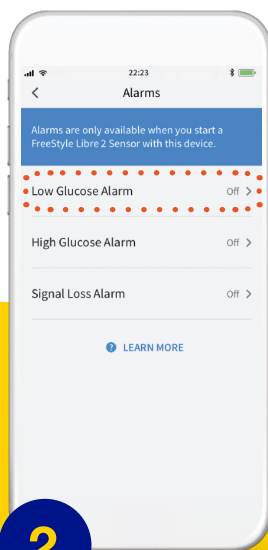



2 Touch **Low Glucose Alarm** and turn on alarm (alarms are off by default)

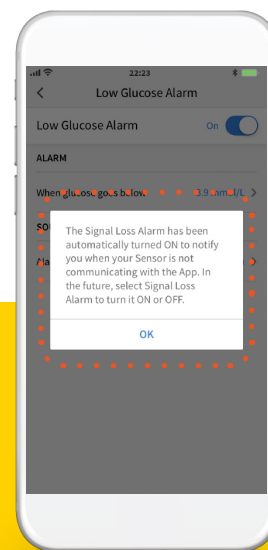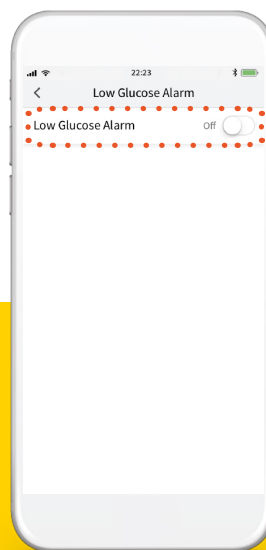


Signal loss alarm is automatically turned on when glucose alarm is turned ON

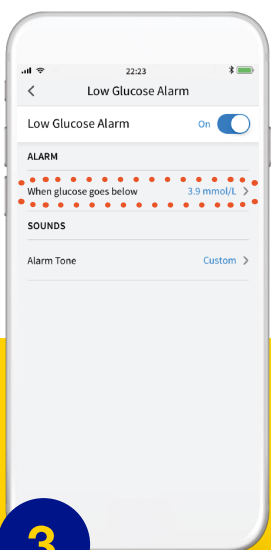

3 Scroll to select **Low Glucose Value**⁴

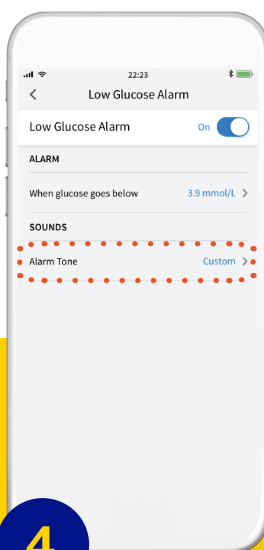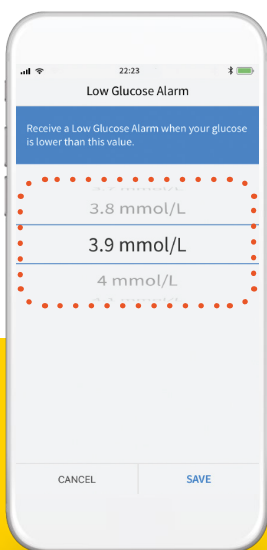

4 Touch **Alarm Tone** and make your tone choice

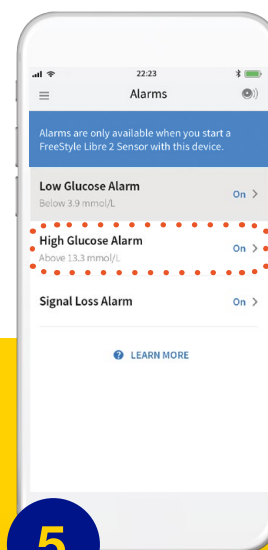

5 Set your **High Glucose Alarm** using the same steps⁵

FreeStyle Libre 2 
FLASH GLUCOSE MONITORING SYSTEM

 **Abbott**
life. to the fullest.®

Images are for illustrative purposes only. Not actual patient data.

1. The FreeStyle LibreLink app is only compatible with certain mobile devices and operating systems. Please check the website for more information about device compatibility before using the app. Use of FreeStyle LibreLink requires registration with LibreView. 2. Scanning the sensor does not require lancets. 3. Please see the FreeStyle LibreLink User's Manual for complete instructions: www.diabetescare.abbott/support/manuals/uk.html 4. 3.9 mmol/L is the default Low Glucose Alarm level and can be set between 3.3-5.6 mmol/L. 5. 13.3 mmol/L is the default High Glucose Alarm level and can be set between 6.7-22.2 mmol/L.

© 2020 Abbott. FreeStyle, Libre, and related brand marks are marks of Abbott. ADC-31515 v1.0 11/20.